



4-Chloromethcathinone

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.



3.2 GAS CHROMATOGRAPHY/MASS SPECTROMETRY


Sample Preparation: Dilute analyte ~3 mg/mL in 1:1 CHCl₃:MeOH.

Instrument: Agilent gas chromatograph operated in split mode with MS detector
Column: DB-5 MS (or equivalent); 30m x 0.25 mm x 0.25 μm
Carrier Gas: Helium at 1 mL/min
Temperatures: Injector: 280°C
MSD transfer line: 280°C
MS Source: 230°C
MS Quad: 150°C
Oven program:
1) 100°C initial temperature for 1.0 min
2) Ramp to 280°C at 12 °C/min
3) Hold final temperature for 9.0 min

Injection Parameters: Split Ratio = 25:1, 1 μL injected
MS Parameters: Mass scan range: 30-550 amu
Threshold: 100
Tune file: stune.u
Acquisition mode: scan

Retention Time: 7.313 min

EI Mass Spectrum: 4-Chloromethcathinone HCl Lot 0465311-20

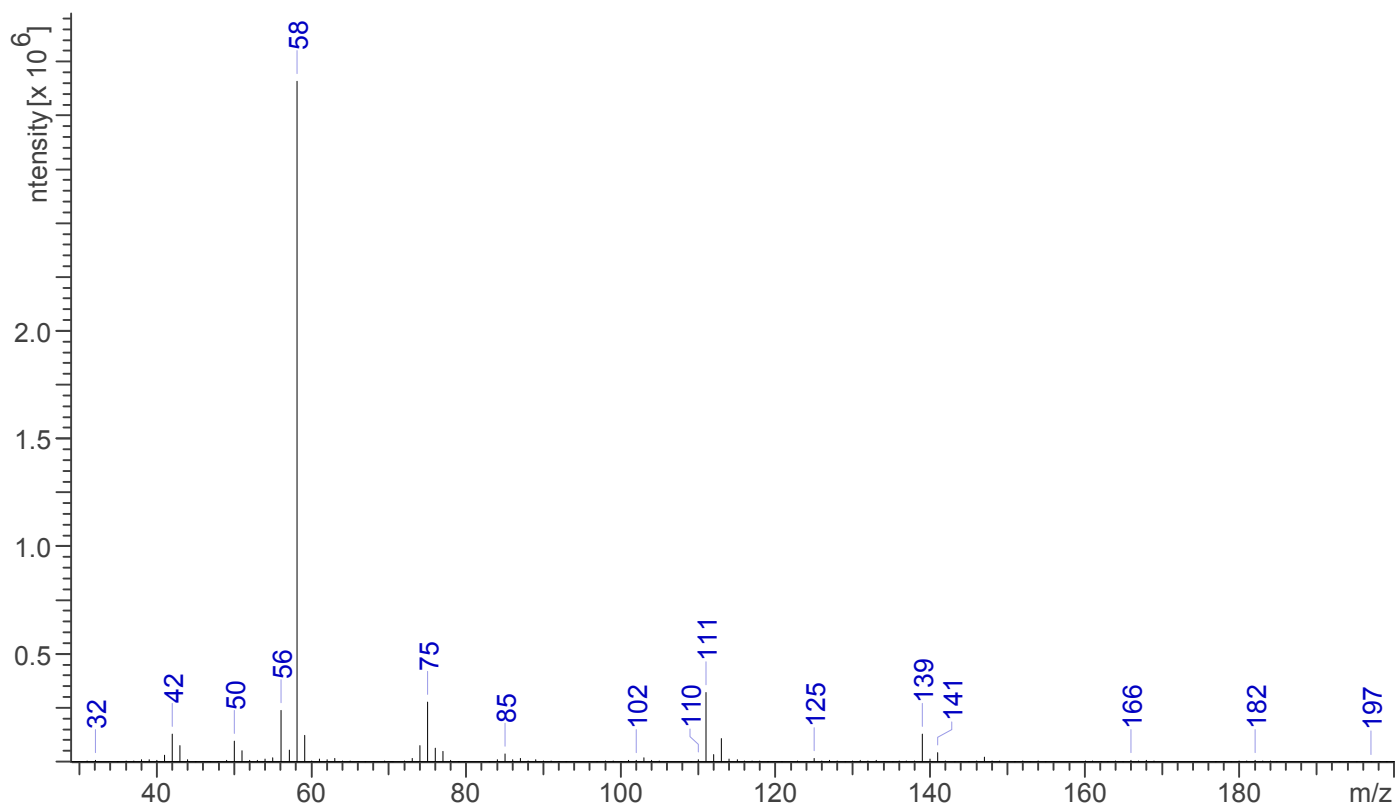



4-Chloromethcathinone

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.





3.3 INFRARED SPECTROSCOPY (FTIR)

Instrument: FTIR with diamond ATR attachment (1 Bounce)

Scan Parameters:
Number of scans: 32
Number of background scans: 32
Resolution: 4 cm⁻¹
Sample gain: 4
Aperture: 80

FTIR ATR (Diamond, 1 Bounce): 4-Chloromethcathinone HCl Lot 0465311-20

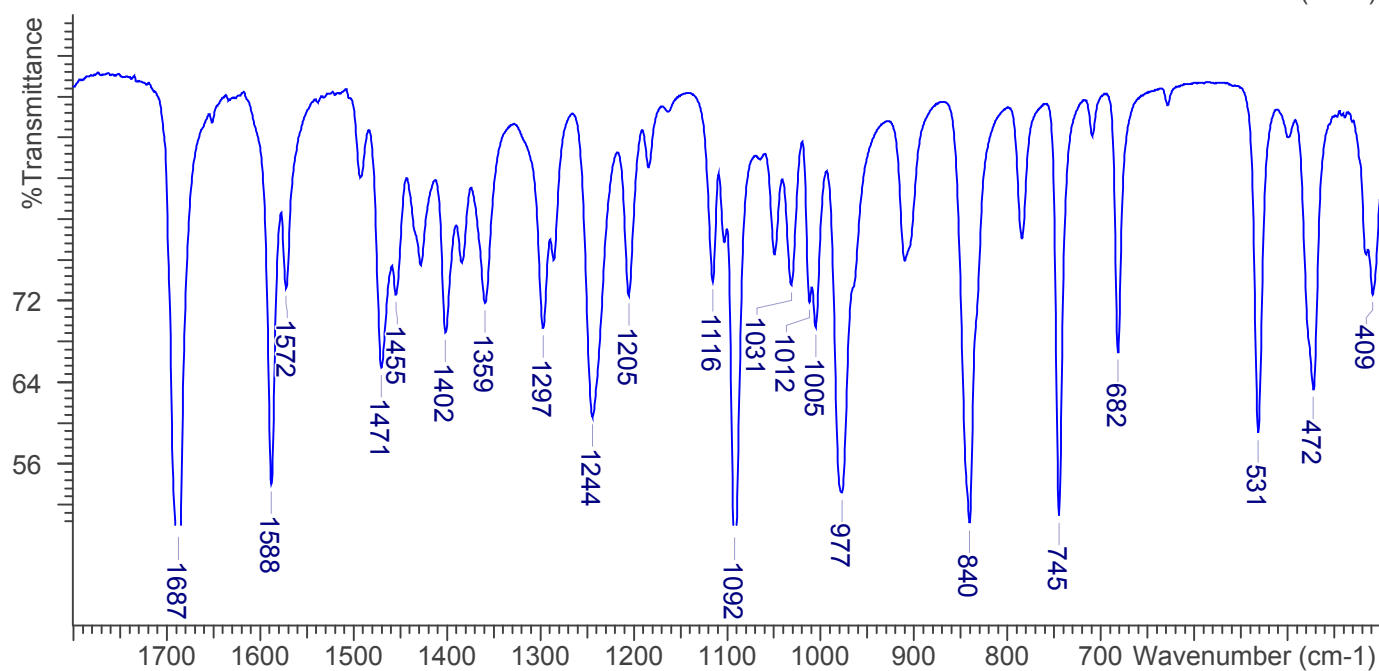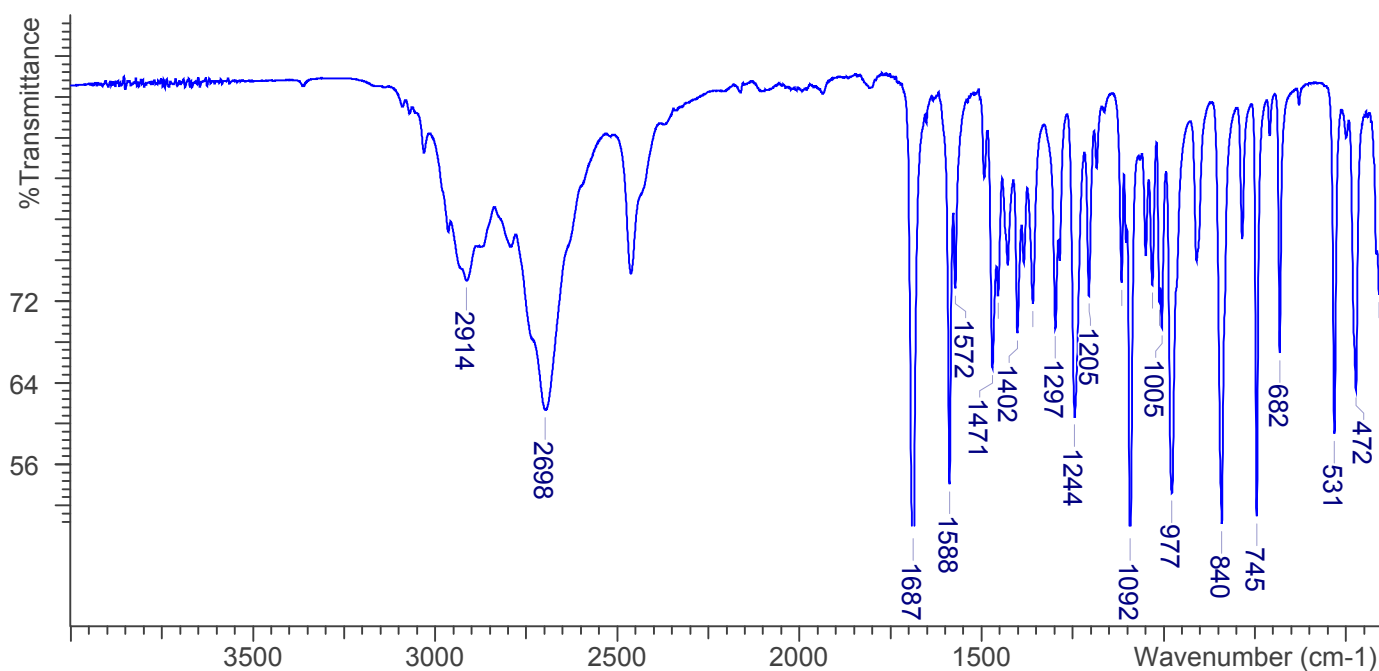



4-Chloromethcathinone

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.



4. ADDITIONAL RESOURCES

[Wikipedia](#)