




Crotonyl fentanyl

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.

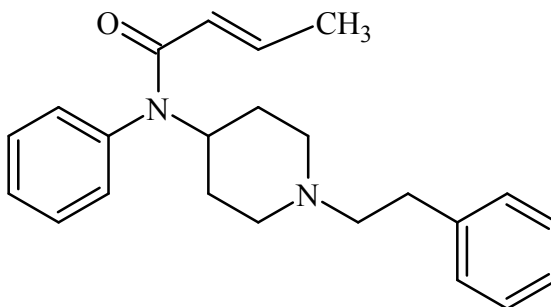

1. GENERAL INFORMATION

IUPAC Name:	(E)-N-(1-phenethylpiperidin-4-yl)-N-phenylbut-2-enamide
CAS#:	760930-59-4 (base)
Synonyms:	(2E)-N-phenyl-N-[1-(2-phenylethyl)piperidin-4-yl]but-2-enamide
Source:	DEA Reference Material Collection
Appearance:	yellow powder
UV_{max}(nm):	NA

2. CHEMICAL AND PHYSICAL DATA

2.1 CHEMICAL DATA

Form	Chemical Formula	Molecular Weight	Melting Point (°C)
Base	C ₂₃ H ₂₈ N ₂ O	348.48	NA



Crotonyl fentanyl

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.




3. QUALITATIVE DATA

3.1 NUCLEAR MAGNETIC RESONANCE

Sample Preparation: Dilute analyte to ~8mg/mL in CD₃OD containing TMS for 0 ppm reference and maleic acid as quantitative internal standard.

Instrument: 400 MHz NMR spectrometer
Parameters: Spectral width: at least containing -3 ppm through 13 ppm
Pulse angle: 90°
Delay between pulses: 45 seconds

¹HNMR: Crotonyl fentanyl; lot# 0511357-12

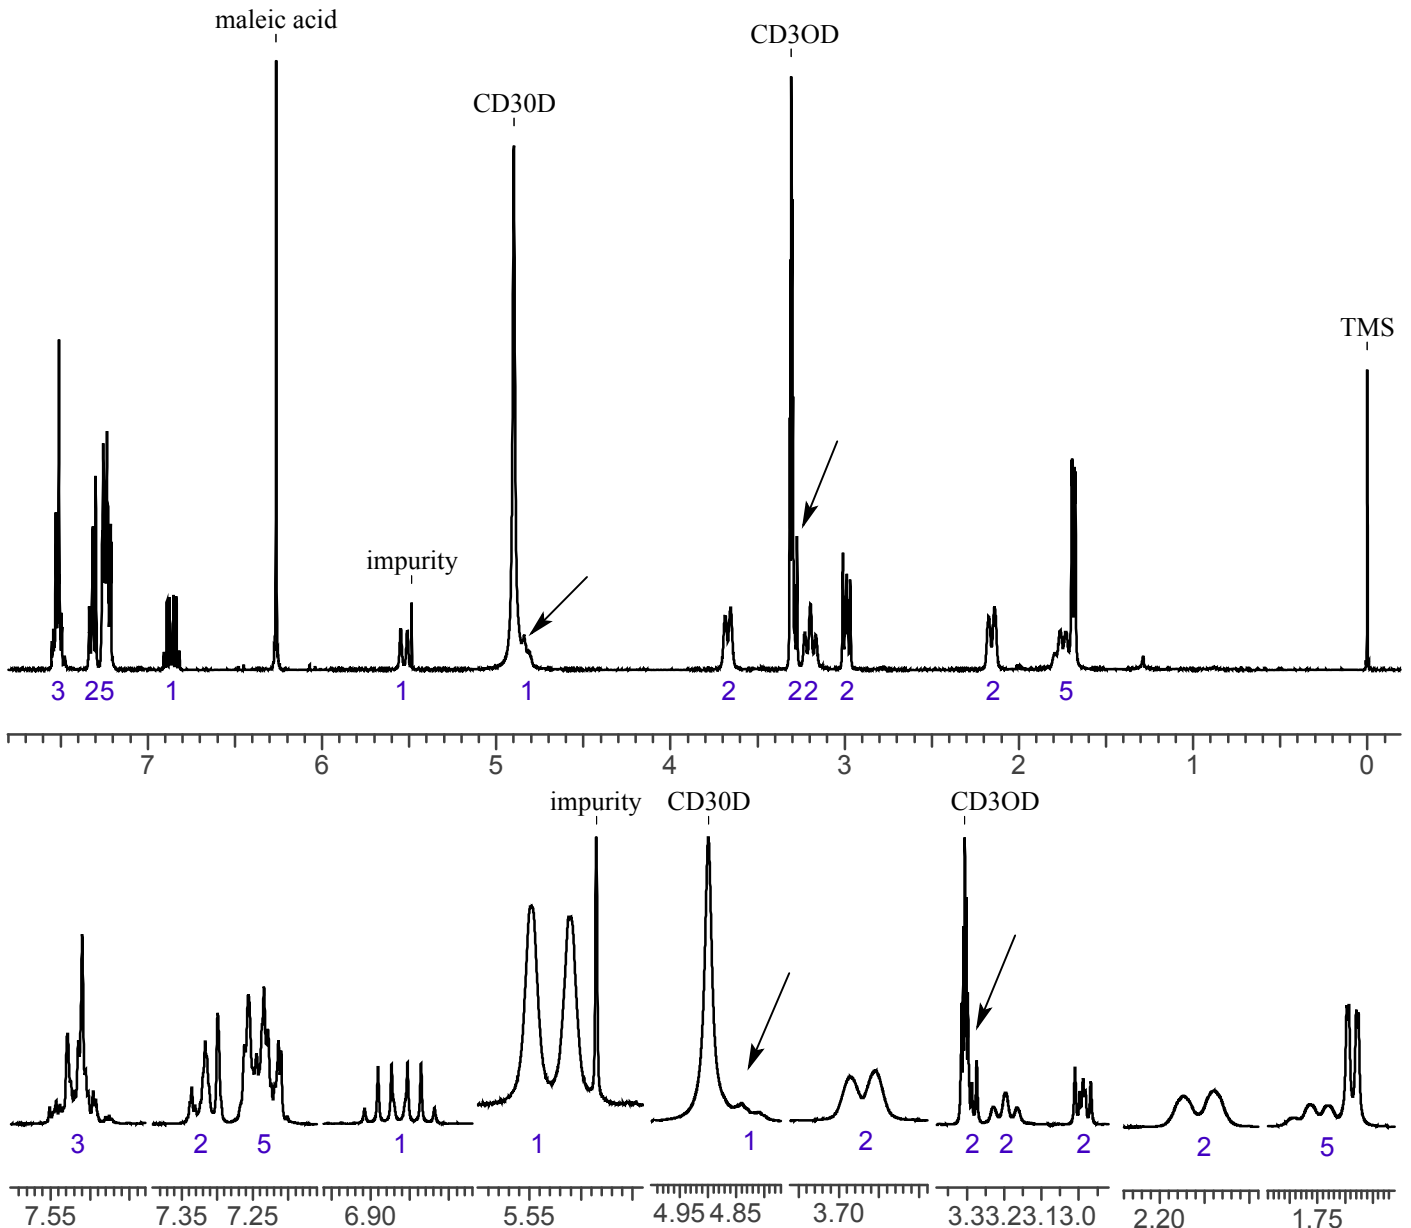



Crotonyl fentanyl

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.



3.2 GAS CHROMATOGRAPHY/MASS SPECTROMETRY

Sample Preparation: Dilute analyte ~4 mg/mL into methanol.

Instrument: Agilent gas chromatograph operated in split mode with MS detector
Column: HP-5; 30m x 0.25 mm x 0.25 μ m
Carrier Gas: Helium at 1.5 mL/min
Temperatures: Injector: 280°C

MSD transfer line: 280°C

MS Source: 230°C

MS Quad: 150°C

Oven program:

1) 100°C initial temperature for 1.0 min

2) Ramp to 280°C at 12 °C/min

3) Hold final temperature for 9.0 min

Injection Parameters: Split Ratio = 25:1, 1 μ L injected

MS Parameters: Mass scan range: 30-550 amu


Threshold: 250

Tune file: stune.u

Acquisition mode: scan

Retention Time: 18.046 min

EI Mass Spectrum: Crotonyl fentanyl; lot# 0511357-12

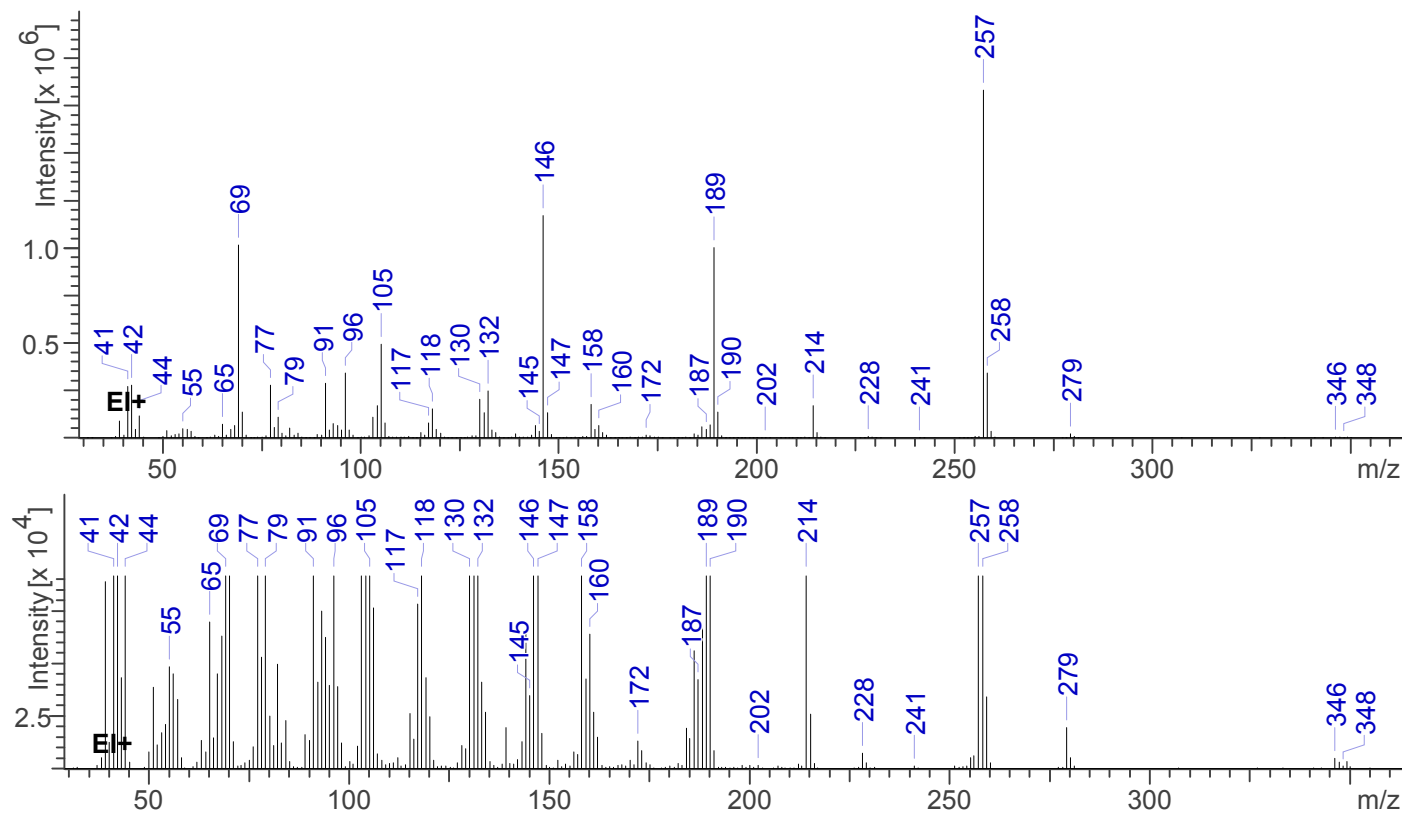



Crotonyl fentanyl



The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.



3.3 INFRARED SPECTROSCOPY (FTIR)

Instrument: FTIR (SensIRDura-Scope ATR Accessory)

Scan Parameters:

Number of scans: 32
Number of background scans: 32
Resolution: 4 cm⁻¹
Sample gain: 1
Aperture: 150

FTIR ATR (Diamond 1 Bounce): Crotonyl fentanyl; lot# 0511357-12

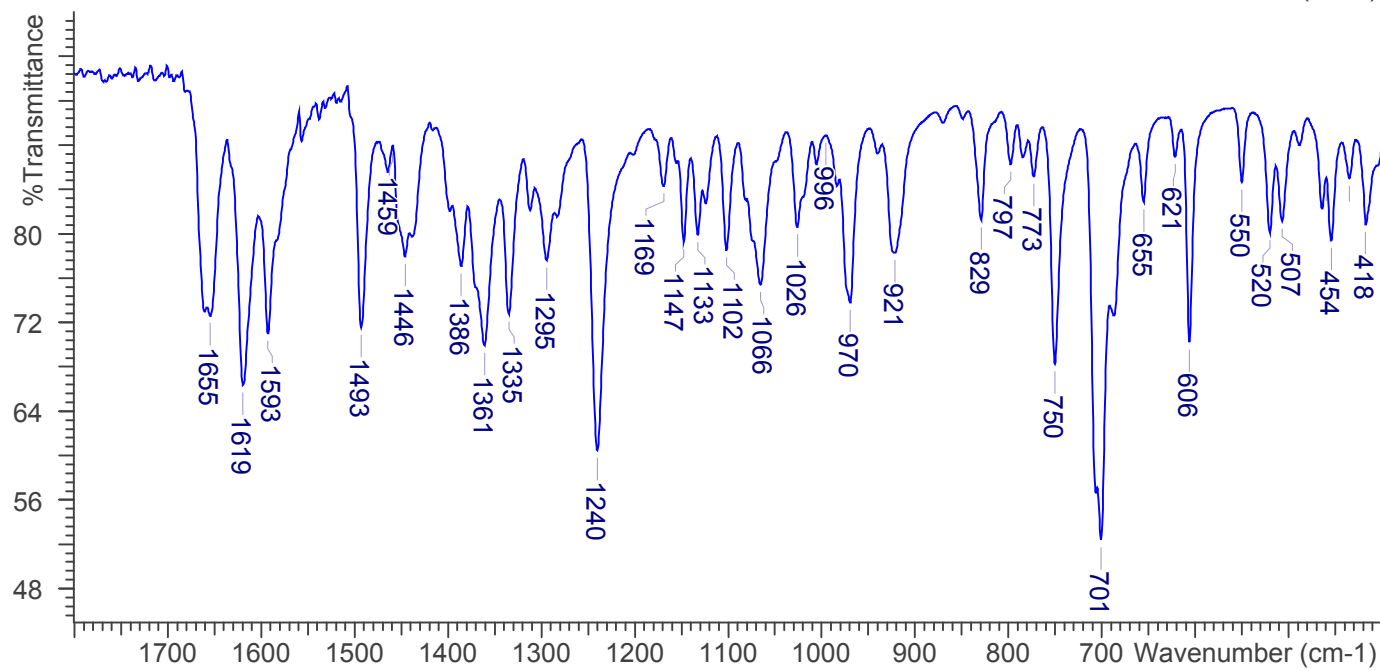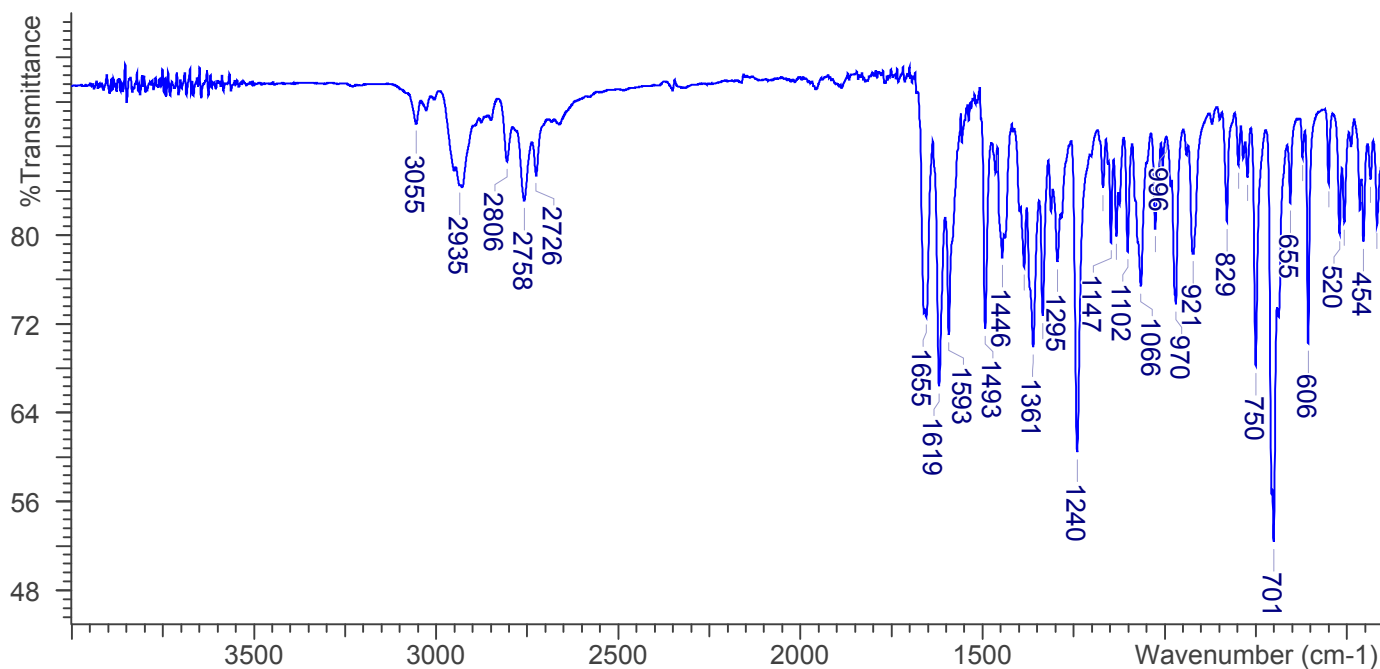



Crotonyl fentanyl

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.



4. ADDITIONAL RESOURCES

no available literature as of 11/08/17