




JWH-022

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.

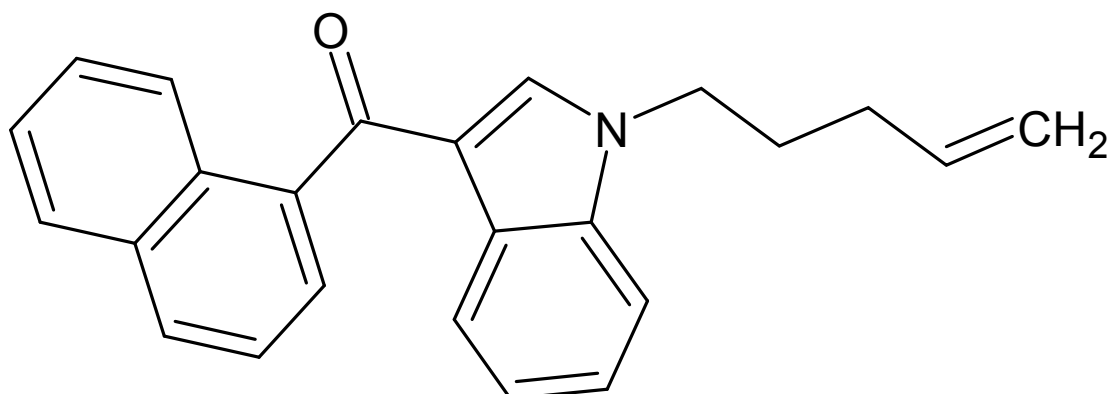

1. GENERAL INFORMATION

| | |
|------------------------------|--|
| IUPAC Name: | naphthalen-1-yl[1-(pent-4-en-1-yl)-1H-indol-3-yl]methanone |
| CAS#: | 209414-16-4 |
| Synonyms: | N/A |
| Source: | DEA Reference Material Collection |
| Appearance: | Light yellow powder |
| UV_{max}(nm): | Not Determined |

2. CHEMICAL AND PHYSICAL DATA

2.1 CHEMICAL DATA

| Form | Chemical Formula | Molecular Weight | Melting Point (°C) |
|------|------------------------------------|------------------|--------------------|
| Base | C ₂₄ H ₂₁ NO | 339 | 56.4 |



JWH-022

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.




3. QUALITATIVE DATA

3.1 NUCLEAR MAGNETIC RESONANCE

Sample Preparation: Dilute analyte to ~10 mg/mL in DMSO-d₆ containing TMS for 0 ppm reference and dimethylfumarate as quantitative internal standard.

Instrument: 400 MHz NMR spectrometer
Parameters: Spectral width: at least containing -3 ppm through 13 ppm
Pulse angle: 90°
Delay between pulses: 45 seconds
¹H NMR: JWH-022 Lot # ALB227-8; DMSO-d₆; 400MHz

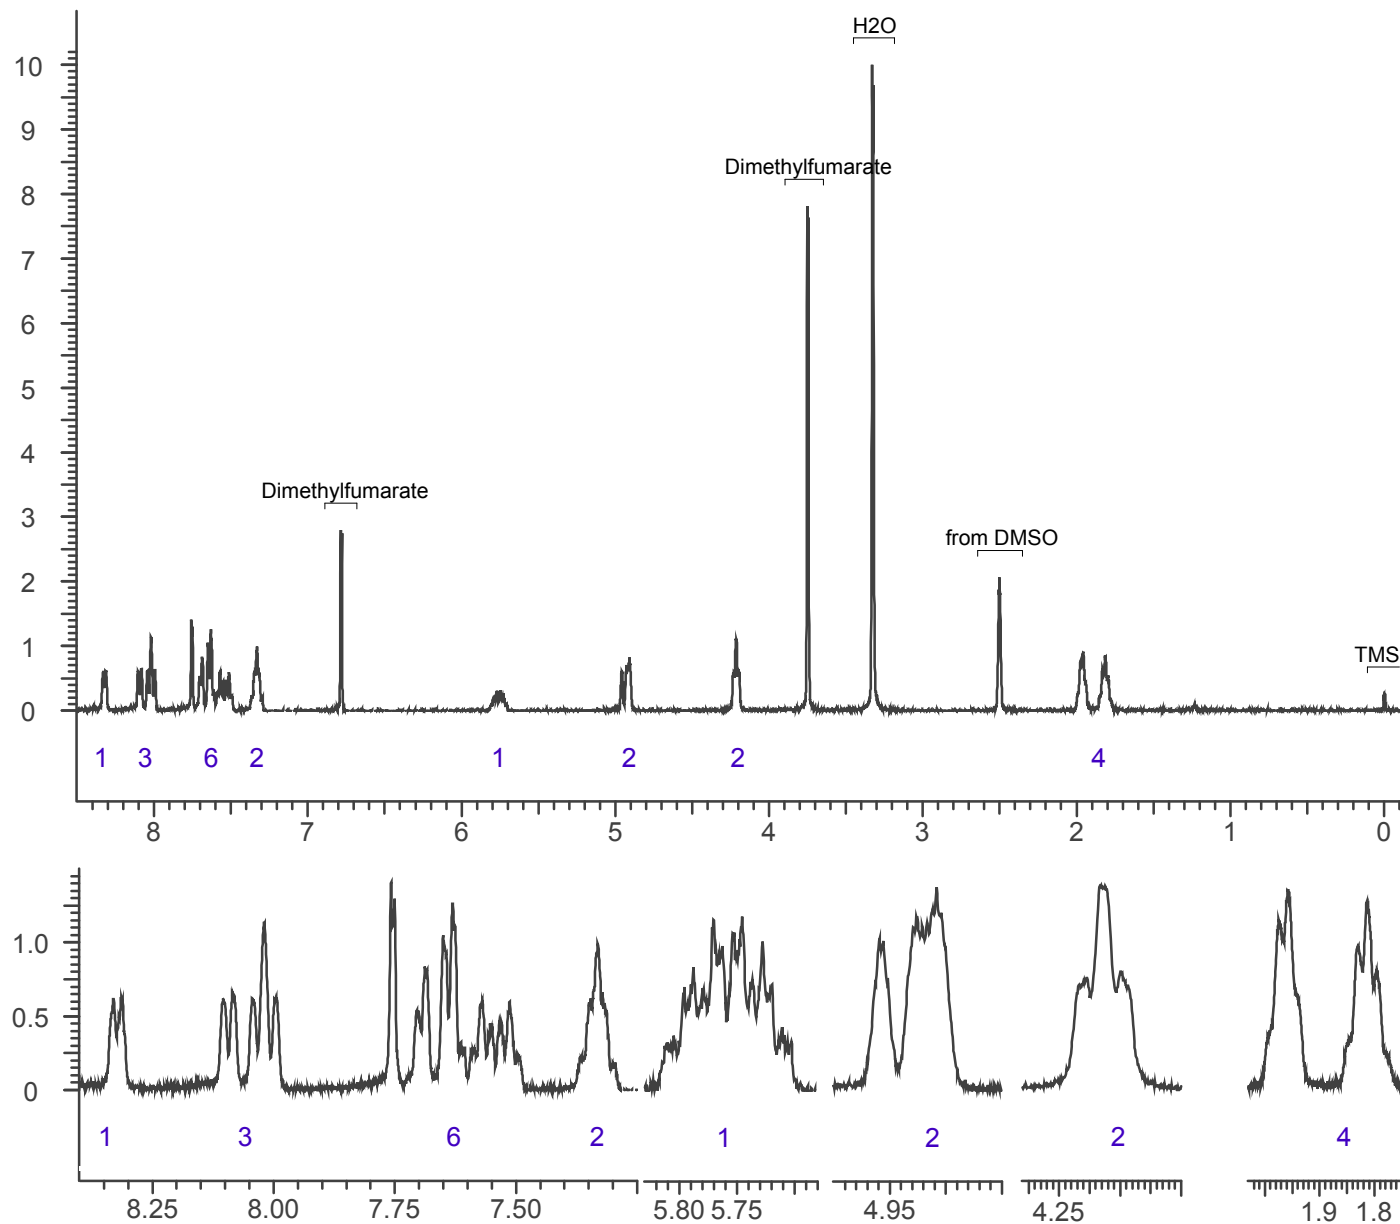



The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.

3.2 GAS CHROMATOGRAPHY/MASS SPECTROMETRY


Sample Preparation: Dilute analyte ~4 mg/mL in methanol.

Instrument: Agilent gas chromatograph operated in split mode with MS detector
Column: DB-1 MS (or equivalent); 30m x 0.25 mm x 0.25 μ m
Carrier Gas: Helium at 1 mL/min
Temperatures: Injector: 280°C
MSD transfer line: 280°C
MS Source: 230°C
MS Quad: 150°C
Oven program:
1) 100°C initial temperature for 1.0 min
2) Ramp to 300°C at 12 °C/min
3) Hold final temperature for 9.0 min

Injection Parameters: Split Ratio = 20:1, 1 μ L injected
MS Parameters: Mass scan range: 30-550 amu
Threshold: 100
Tune file: stune.u
Acquisition mode: scan

Retention Time: 20.370 min

EI Mass Spectrum: JWH-022 Lot # ALB227-8

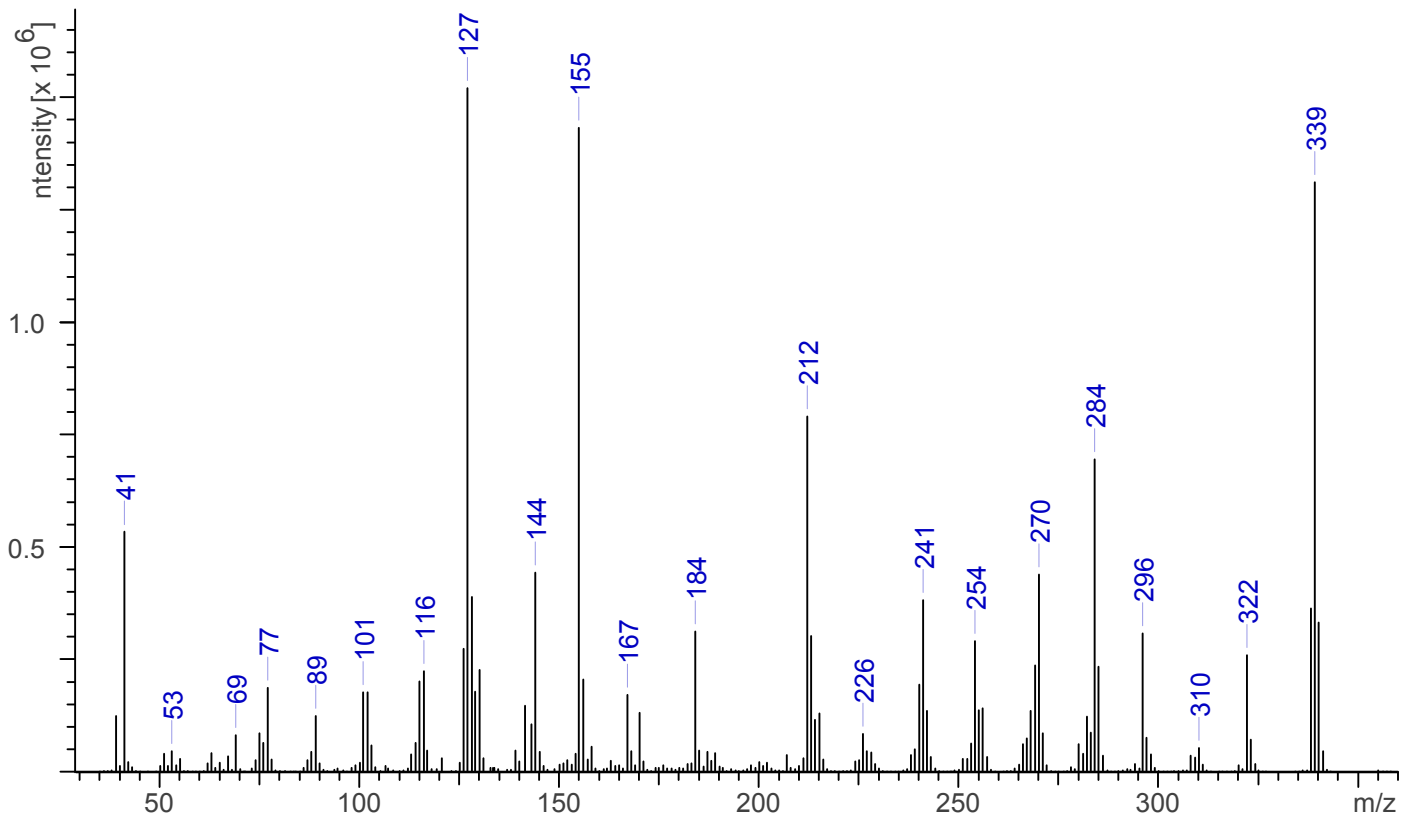





3.3 INFRARED SPECTROSCOPY (FTIR)

Instrument: FTIR with diamond ATR attachment (3 bounce)

Scan Parameters: Number of scans: 32
Number of background scans: 32
Resolution: 4 cm⁻¹
Sample gain: 8
Aperture: 150

FTIR ATR (Diamond, 3 Bounce): JWH-022 Lot # ALB227-8

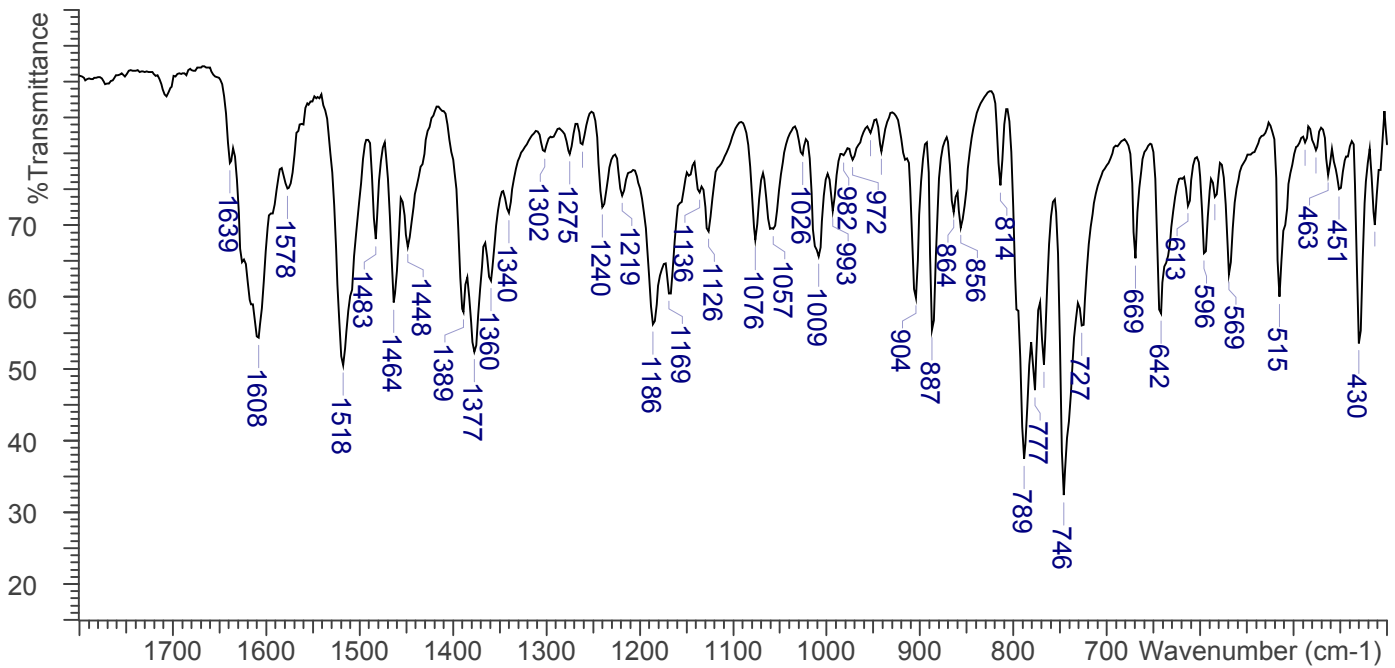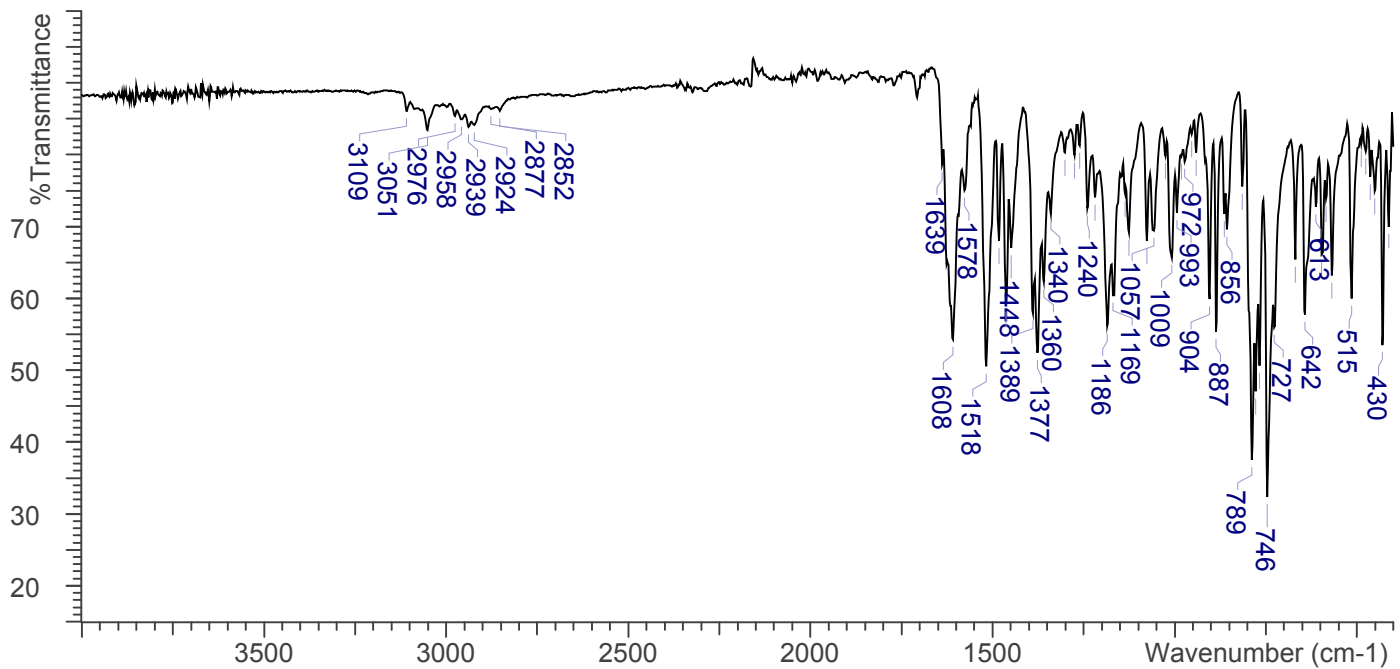



JWH-022

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.



4. ADDITIONAL RESOURCES

[Forendex](#)

[Wikipedia](#)