









# ortho-Fluorofentanyl

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.





## 3.3 INFRARED SPECTROSCOPY (FTIR)

**Instrument:** FTIR with diamond ATR attachment (1 bounce)

**Scan Parameters:**  
Number of scans: 32  
Number of background scans: 32  
Resolution: 4 cm<sup>-1</sup>  
Sample gain: 4  
Aperture: 80

FTIR ATR (Diamond 1 Bounce): ortho-Fluorofentanyl HCl; LOT # RM-160713-01

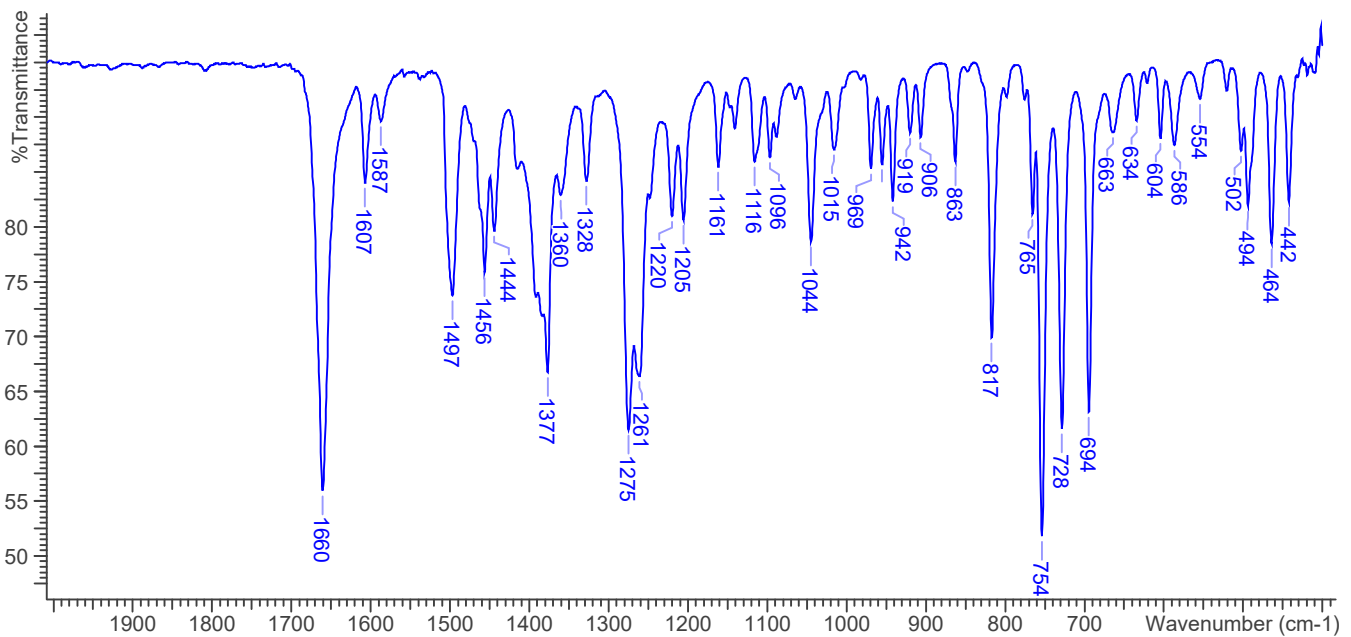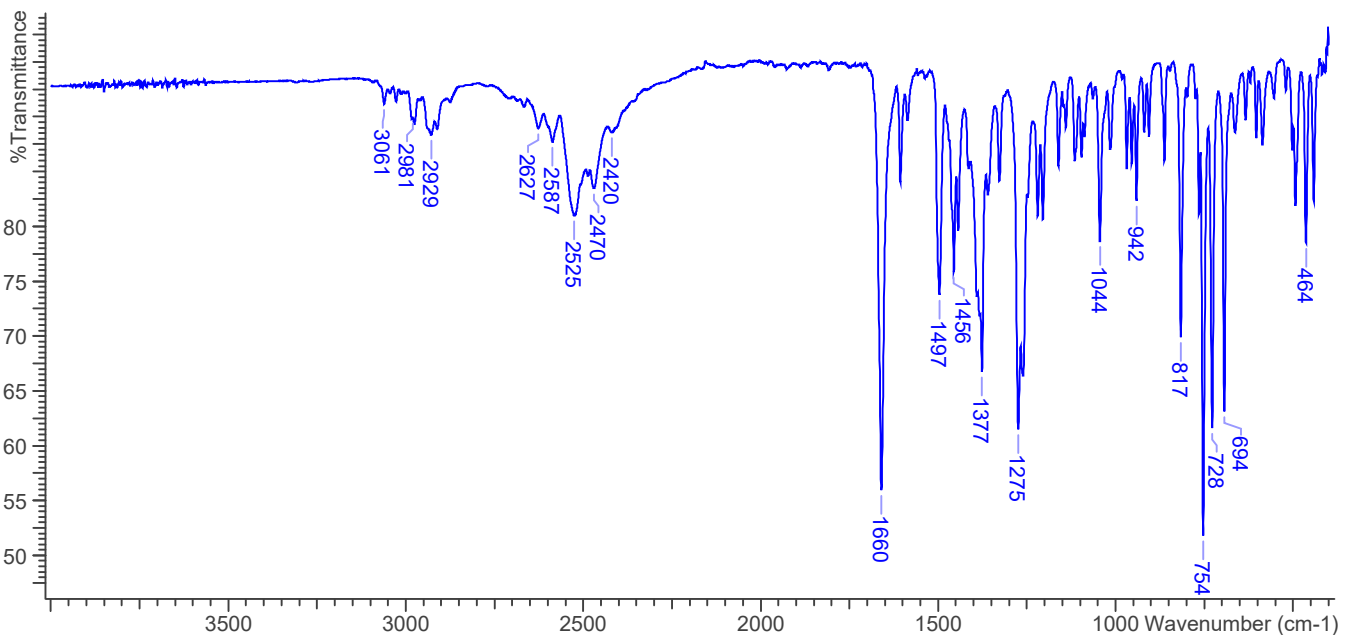



## ortho-Fluorofentanyl

*The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.*



### **4. ADDITIONAL RESOURCES**

No additional resources as of 09/2016