




2C-B-BZP

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.

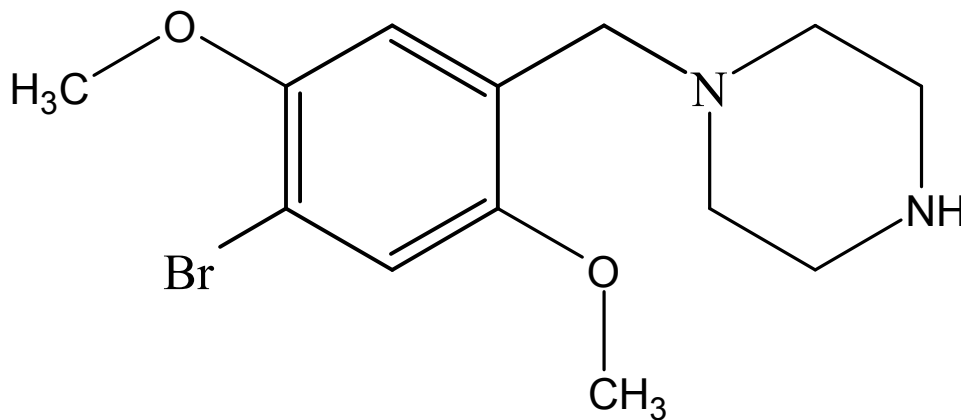

1. GENERAL INFORMATION

IUPAC Name: 1-(4-bromo-2,5-dimethoxybenzyl)piperazine

CAS#: Not Available

Synonyms: 4-bromo-2,5-dimethoxybenzylpiperazine;
4-bromo-2,5-dimethoxy-1-benzylpiperazine

Source: DEA Reference Material Collection

Appearance: White powder (di-HCl)

UV_{max}(nm): Not Determined

2. CHEMICAL AND PHYSICAL DATA

2.1 CHEMICAL DATA

Form	Chemical Formula	Molecular Weight	Melting Point (°C)
Base	C ₁₃ H ₁₉ BrN ₂ O ₂	315	Not Determined
di-HCl	C ₁₃ H ₁₉ BrN ₂ O ₂ · 2HCl	388	Not Determined



2C-B-BZP

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.



3. QUALITATIVE DATA


3.1 NUCLEAR MAGNETIC RESONANCE

Method NMR D₂O

Sample Preparation: Dilute analyte to ~10 mg/mL in D₂O containing TSP for 0 ppm reference and maleic acid as quantitative internal standard.

Instrument: 400 MHz NMR spectrometer
Parameters: Spectral width: at least containing -3 ppm through 13 ppm
Pulse angle: 90°
Delay between pulses: 45 seconds

¹H NMR: 2C-B BZP di-HCl Lot # H-0416

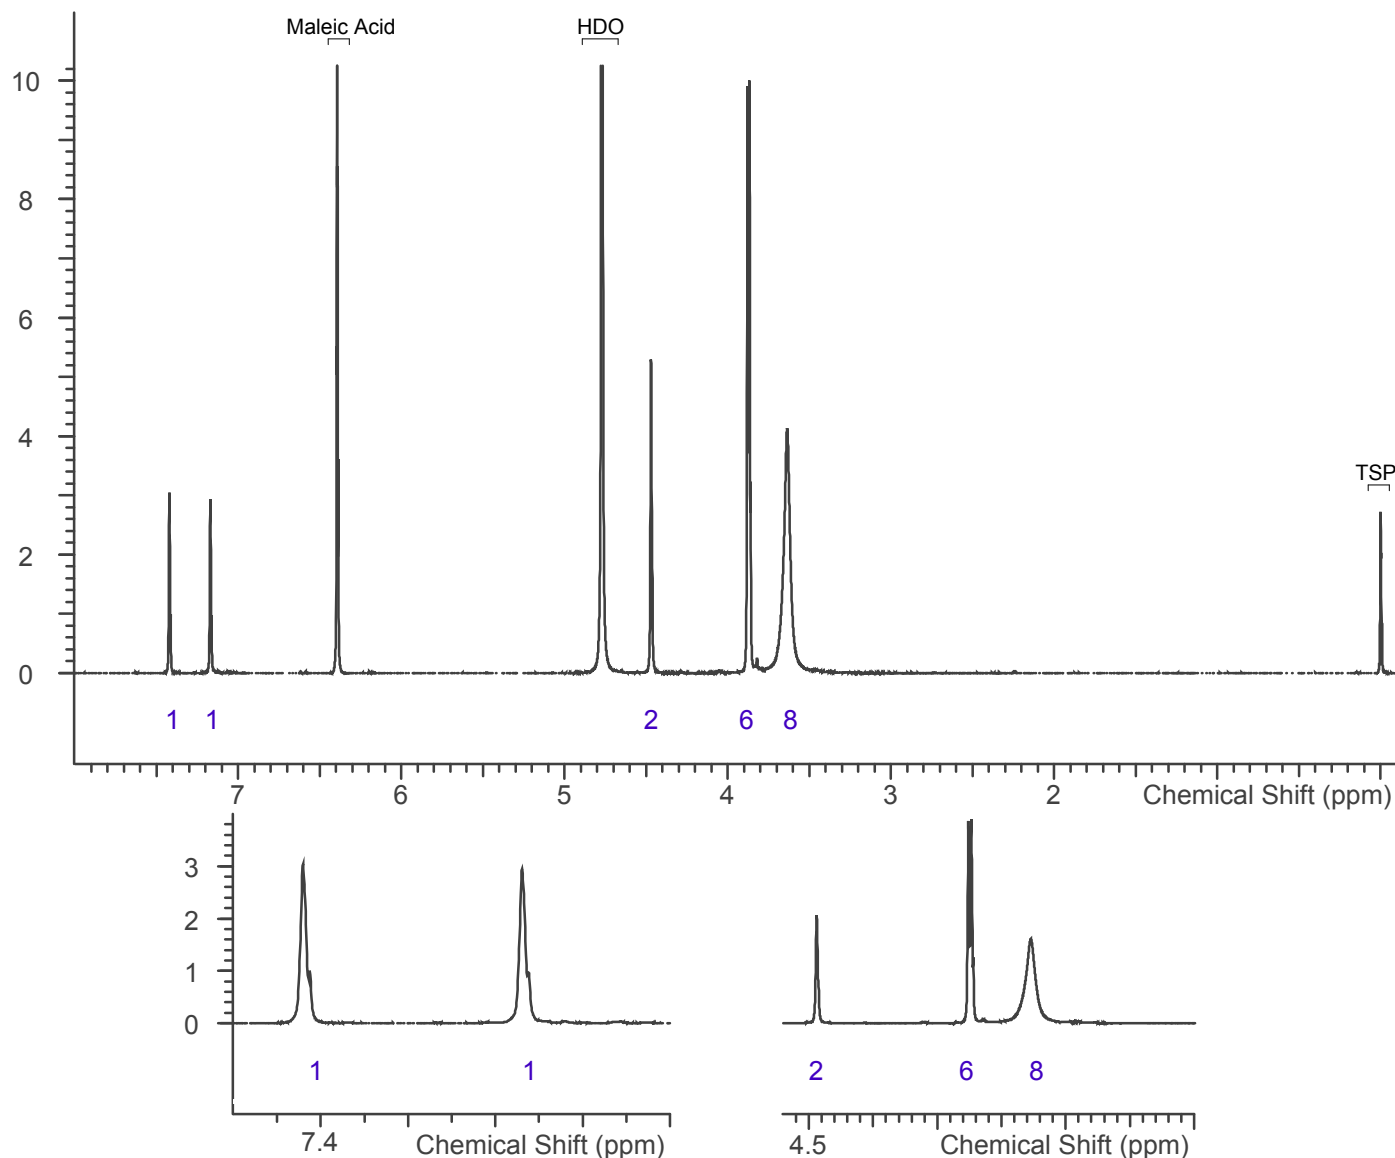



2C-B-BZP

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.



3.2 Gas Chromatography/Mass Spectrometry

Sample Preparation: Dilute analyte ~1 mg/mL base extracted into chloroform.

Instrument: Agilent gas chromatograph operated in split mode with MS detector

Column: DB-1 MS (or equivalent); 30m x 0.25 mm x 0.25 μ m

Carrier Gas: Helium at 1 mL/min

Temperatures: Injector: 280°C
MSD transfer line: 280°C

MS Source: 230°C

MS Quad: 150°C

Oven program:

1) 100°C initial temperature for 1.0 min

2) Ramp to 300°C at 12 °C/min

3) Hold final temperature for 9.0 min

Injection Parameters: Split Ratio = 20:1, 1 μ L injected

MS Parameters: Mass scan range: 30-550 amu


Threshold: 100

Tune file: stune.u

Acquisition mode: scan

Retention Time: 13.502 min

EI Mass Spectrum: 2C-B BZP di-HCl Lot # H-0416

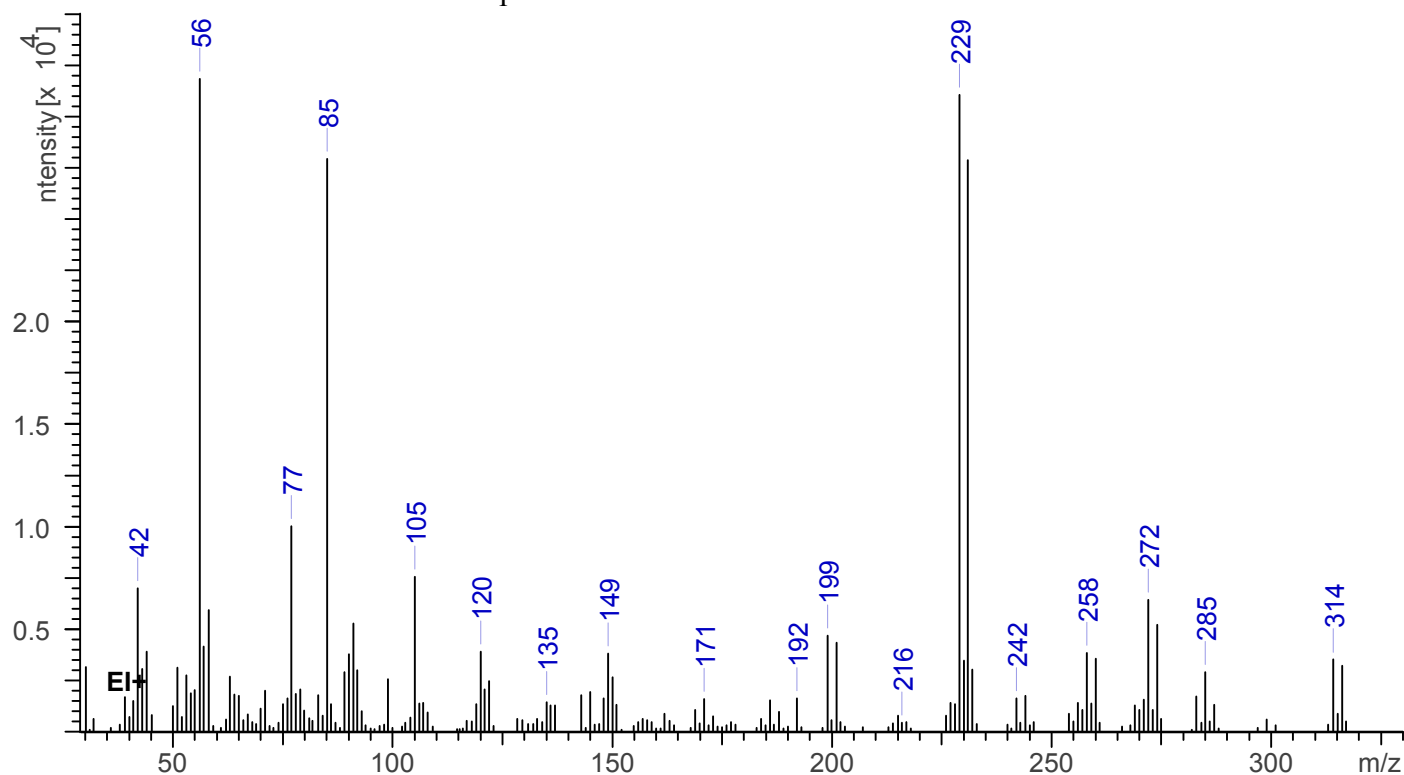



2C-B-BZP

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.





3.3 INFRARED SPECTROSCOPY (FTIR)

Instrument: FTIR with diamond ATR attachment (3 bounce)

Scan Parameters:
Number of scans: 32
Number of background scans: 32
Resolution: 4 cm⁻¹
Sample gain: 8
Aperture: 150

FTIR ATR (Diamond, 3 Bounce): 2C-B BZP di-HCl Lot # H-0416

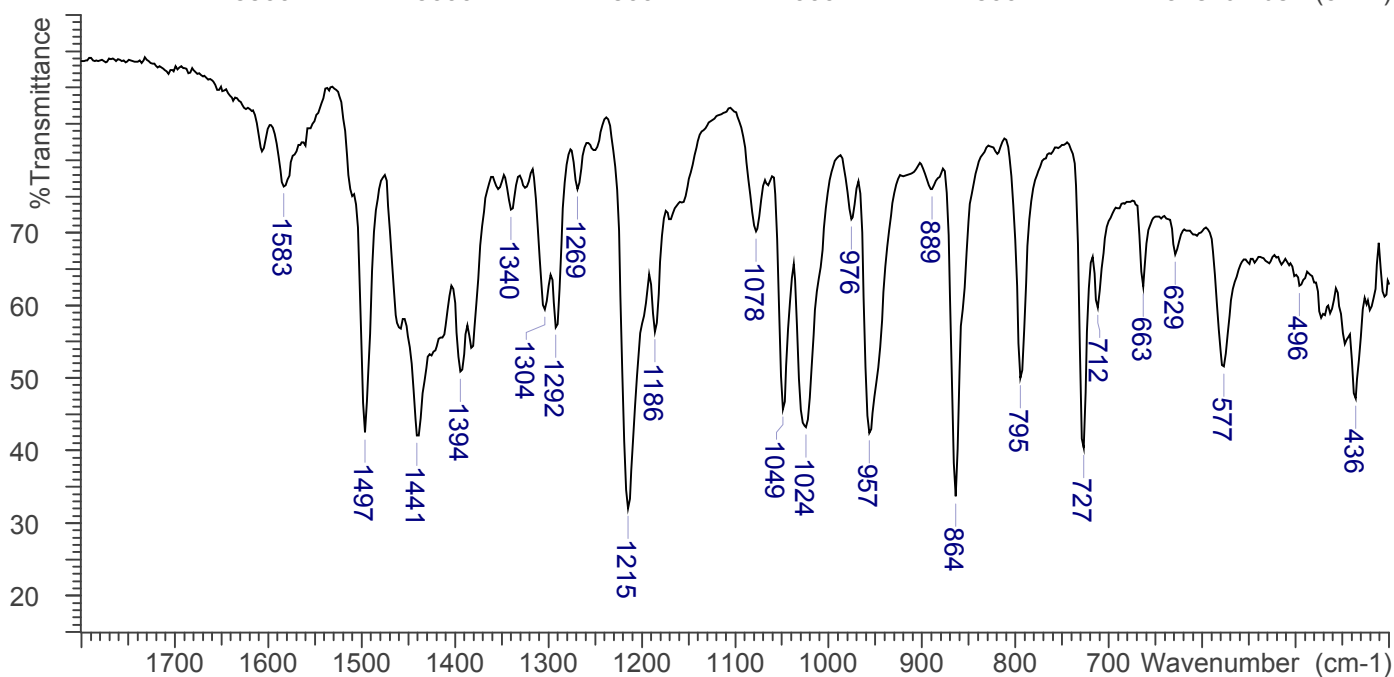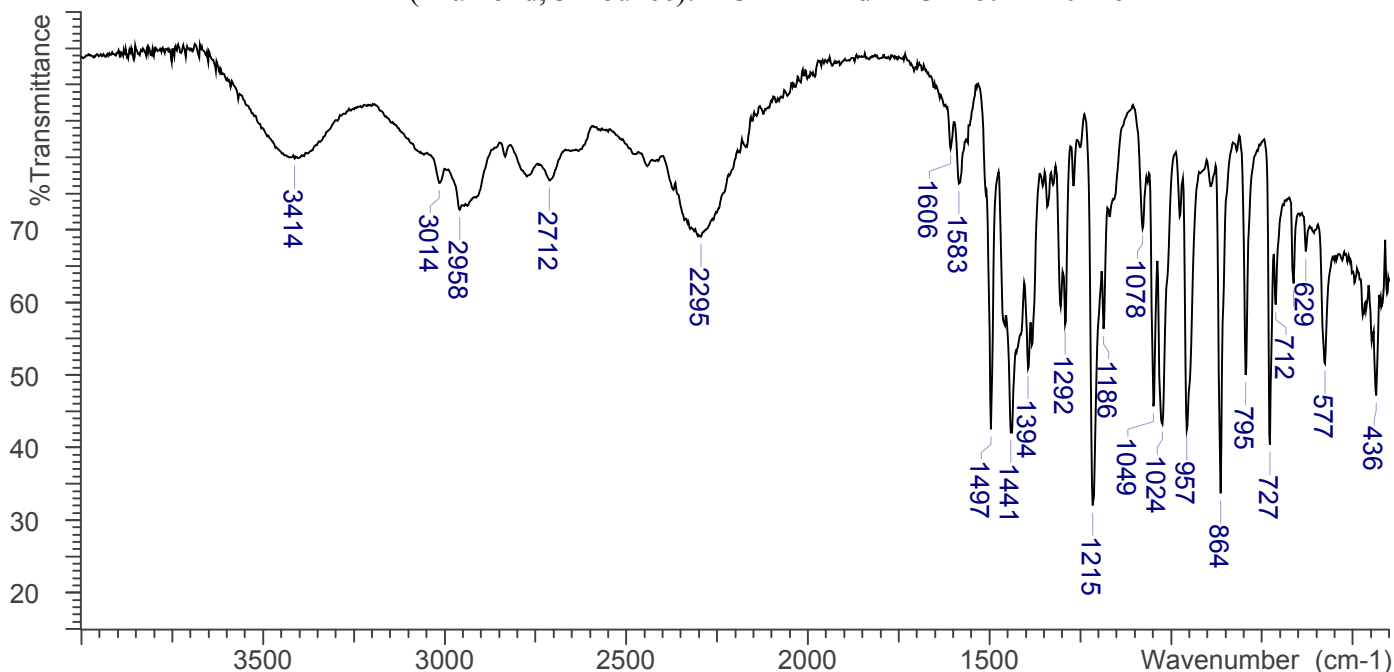



2C-B-BZP

The Drug Enforcement Administration's Special Testing and Research Laboratory generated this monograph using structurally confirmed reference material.



4. ADDITIONAL RESOURCES

[Wikipedia](#)